Biomedical Optics

Biomedical Optics. SPIE Digital Library. org

Use of combined polarization-sensitive optical coherence tomography and Mueller matrix imaging for the polarimetric characterization of excised biological tissue (Erratum)

Joseph Chue-Sang Yuqiang Bai Susan Stoff David Straton Sharan Ramaswamy Jessica C. Ramella-Romana



Use of combined polarization-sensitive optical coherence tomography and Mueller matrix imaging for the polarimetric characterization of excised biological tissue (Erratum)

Joseph Chue-Sang,^a Yuqiang Bai,^a Susan Stoff,^a David Straton,^a Sharan Ramaswamy,^a and Jessica C. Ramella-Romana^b

^aFlorida International University, Department of Biomedical Engineering, 10555 West Flagler Street, EC 2600, Miami, Florida 33174, United States ^bFlorida International University, Herbert Wertheim College of Medicine, 11200 SW 8th Street, AHC2, Miami, Florida 33199, United States

[DOI: 10.1117/1.JBO.22.10.109801]

This article [*J. Biomed. Opt.* **21**(7), 071109 (2016)] was originally published online on 1 March 2016 with two errors, described below.

On p. 3, there is an error in a value in the Mueller matrix. In column 2, row 2, 0.100 has been changed to 1.000 as shown:

In addition, Fig. 1 showed an extra component, the quarterwavelength plate (QWP), which has been removed from the diagram.

This article was corrected online on 14 October 2017.

$$\begin{bmatrix} 0.997 & -0.000 & 0.001 & -0.005 \\ 0.004 & 1.000 & 0.010 & -0.001 \\ -0.001 & 0.004 & 0.991 & 0.002 \\ 0.001 & -0.002 & 0.009 & 0.999 \end{bmatrix}$$

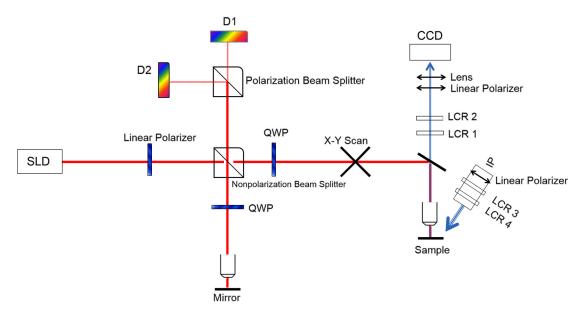


Fig. 1 Combined PS-OCT and Mueller matrix polarimeter schematic.